


<b>Name of Policy:</b> Dry-Run on EDGE linear accelerator		 <b>Original effective date:</b> <b>5/2015</b>
<b>Policy Number:</b> 3364-134-105		
<b>Approving Office:</b> Chief Operating & Clinical Officer Professor & Chairman, Radiation Oncology		
<b>Responsible Agent:</b> Technical Manager, Radiation Oncology		
<b>Scope:</b> Radiation Oncology		
X	New policy proposal	Minor/technical revision of existing policy
	Major revision of existing policy	Reaffirmation of existing policy

(A) Policy statement


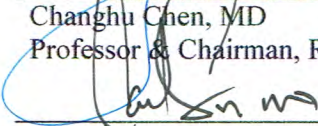
A dry run will be performed on all patients pre-treatment on the EDGE linear accelerator.

(B) Purpose of policy

To ensure that the machine in which the treatment planned for the patient clears the patient, and table. Guarantee that no collisions will occur.

(C) Procedure

- Set the patient up on the treatment table.
- Make sure that the CBCT clears prior imaging.
- Check all angles of planned treatment fields.
- If patients' treatment plan is checked and all clearance is confirmed, therapists may rotate the table from outside the treatment room.

<b>Approved by:</b>  <hr/> Changhu Chen, MD Professor & Chairman, Radiation Oncology  <hr/> Carl Sirio, MD Chief Operating & Clinical Officer  <i>Review/Revision Completed By:</i> Michelle Giovanoli	Date: <u>5/13/2015</u> Date: <u>5/20/15</u>	<b>Review/Revision Date:</b>          <b>Next Review Date:</b> 5/2018
---	--	---